

ARMY RESEARCH LABORATORY



A New Technique for the Simultaneous Measurement of Thermal Diffusivity and Thermal Conductivity of Small Energetic-Material Specimens

by Martin S. Miller
and Anthony J. Kotlar

ARL-TR-1321

March 1997

19970321 084

Approved for public release; distribution is unlimited.

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

Citation of manufacturer's or trade names does not constitute an official endorsement or approval of the use thereof.

Destroy this report when it is no longer need. Do not return it to the originator.

Army Research Laboratory

Aberdeen Proving Ground, MD 21005-5066

ARL-TR-1321

March 1997

A New Technique for the Simultaneous Measurement of Thermal Diffusivity and Thermal Conductivity of Small Energetic-Material Specimens

Martin S. Miller, Anthony J. Kotlar
Weapons and Materials Research Directorate, ARL

Approved for public release; distribution is unlimited.

DTIC QUALITY INSPECTED 3

Abstract

An experimental technique to simultaneously measure the thermal diffusivity and thermal conductivity of small specimens of thermal-insulator materials is described. Experimental conditions that approach the mathematical idealization of a one-dimensional, infinite, two-component, composite solid whose planar interface is subjected to a step-function heat flux are developed. The heat flux is generated by resistive heating of a thin metallic foil. Although this principle has been exploited previously, the present technique permits specimens with volumes two orders of magnitude smaller than prior work based on the same idealization. A number of difficulties related to small specimen volume are identified and overcome. Another improvement over past efforts is the use of nonlinear least-squares analysis to determine the optimum values for diffusivity and conductivity. A comparison of measurements of these properties for acrylic and Pyrex glass with literature values suggests that the technique affords accuracies of about 5% for materials in this range.

TABLE OF CONTENTS

		<u>Page</u>
	LIST OF FIGURES	v
	LIST OF TABLES	vii
1.	INTRODUCTION	1
2.	IDEALIZATION	3
3.	EXPERIMENTAL ARRANGEMENT	4
4.	EXPERIMENTAL CONDITIONS FOR SATISFYING THE IDEALIZATION	6
4.1	Step-Function Flux	6
4.2	Uniformity of Flux	8
4.3	Semi-Infinite Specimen	10
4.4	Instrumentation Issues	12
5.	DATA ANALYSIS	13
6.	DIFFUSIVITY RESULTS	15
7.	REFERENCES	19
	DISTRIBUTION LIST	21
	REPORT DOCUMENTATION PAGE	27

INTENTIONALLY LEFT BLANK

LIST OF FIGURES

<u>Figure</u>	<u>Page</u>
1. Schematic of thermal diffusivity/conductivity fixture in cross-sectional view.....	4
2. Measurements of total electrical resistance of series circuit containing Constantan foil and contact resistances between foil and terminal blocks for foils of varying lengths. Total electrical contact resistance is the y-intercept of the least-squares fit (solid line)	7
3. Worst-case calculations of nonuniformity in foil temperature due to heat losses to terminal blocks at the ends of the foil. Temperatures are expressed as a fraction of the temperature of the foil if there were no heat losses. Nonuniformities in foil temperature over the region occupied by the specimen will result in spatial nonuniformity of the heat flux, invalidating the mathematical idealization	9
4. Worst-case calculations of departures from one-dimensionality of the temperature field in the specimen due to the finite width of the foil for two different specimen materials. Calculated is the temperature generated at a point along an axis through a disk source of diameter equal to the width of the foil. The results are displayed as a fraction of the temperature generated by a planar source of infinite extent	10
5. Calculations of the minimum thickness of a specimen (wafer + back-up piece) for which the temperature at a distance from the foil equal to the indicated wafer thickness differs from the temperature that would result from an infinite-thickness specimen by 1%. The figure shows, for example, that a total specimen thickness of 0.6 cm is sufficiently thick to approximate being infinitely thick in testing a material with a thermal diffusivity of $0.01 \text{ cm}^2/\text{s}$ if the data acquisition time is 10 s (or less). Vertical decade grid lines are shown for convenience	11
6. Typical experimental temperature data (points) measured for an acrylic (PMMA) specimen at a distance of 0.052 cm from the foil compared with the theoretical temperature (solid curve) computed from Equation (6) with the optimized values for thermal conductivity and diffusivity	14

INTENTIONALLY LEFT BLANK

LIST OF TABLES

<u>Table</u>	<u>Page</u>
1. Results of present technique compared to published work on similar materials	16

INTENTIONALLY LEFT BLANK

1. INTRODUCTION

In connection with a program to measure and interpret temperature profiles in deflagrating propellants, there arose a need in our laboratory for the measurement of thermal conductivity using small specimens of solid propellant with dimensions of the order of half a centimeter. Steady-state measurements of thermal conductivity by the guarded-hot-plate method typically employ specimens as much as a hundred times larger¹ and are time-consuming because of the time required to establish steady-state conditions at each test temperature. As have many before us, we chose rather to pursue a transient-response experiment which, in addition to mitigating the drawbacks of the steady-state method, offers the advantage of simultaneously determining both the thermal diffusivity and thermal conductivity. This report describes the development of the technique and discusses the experimental subtleties arising from the use of such small specimens.

In measurements of thermal diffusivity, experimental conditions are usually arranged to approach the set of boundary conditions for which an exact solution is available to the following approximate form of the time-dependent, one-dimensional, heat-conduction equation:

$$\frac{\partial T}{\partial t} = \alpha \frac{\partial^2 T}{\partial x^2}, \quad (1)$$

where α is the thermal diffusivity, T the temperature, x the spatial coordinate, and t the time. In addition to having to satisfy the boundary conditions, the temperature range encompassed by the experiment must be small enough to neglect temperature variations of both the thermal conductivity (a condition required for validity of Equation (1)) and diffusivity (required for the validity of practically all the exact solutions).

In the flash method², for instance, the experiment is intended to simulate a homogeneous, insulated, finite-thickness slab of specimen material of infinite lateral extent, one face of which is instantaneously elevated in temperature. The temperature increase is accomplished by exposing the sample, whose face is blackened to boost the amount of energy absorbed, to the radiant output of a

flash tube or pulsed laser. Developed for metals, the experimental times are short enough that conductive and convective heat losses at the sample boundaries can be ignored. Radiative heat losses are important at high temperatures, and correction strategies have been discussed by Clark and Taylor³. Conduction and convection losses at the sample boundary are important for low-diffusivity materials but can be virtually eliminated by placing the sample in a vacuum chamber⁴. The method has been found suitable for sample sizes down to 6 mm.

A simpler experimental setup was used by Plummer, et al.⁵ for various glasses/ceramics and by Harmathy⁶ for building materials such as bricks and concrete blocks. Both articles describe the use of resistively heated metal foils in an arrangement intended to approximate a semi-infinite, one-dimensional solid whose surface is subjected to a constant, spatially uniform heat flux of sudden onset. Both studies also used specimens whose lateral dimensions were on the order of 10 cm. The choices of experiment duration, temperature-sampling distance, foil thickness, heating power, etc. were conditioned by the availability of relatively large specimens and the desire to minimize errors in the diffusivity measurement. Steere⁷ showed that Harmathy's technique could be extended to specimens consisting of multilayers of thin-film polymers and to specimens about two orders of magnitude smaller in volume, mainly by using very thin metal foils. In this paper we further extend the technique to specimens about two orders of magnitude smaller in volume than those used by Steere⁷.

The present effort was undertaken in the belief that a heated-foil source would require less sample-preparation labor and utilize more readily available equipment than the radiant flash method. First efforts concentrated on impulse heating of the ribbon by capacitor discharge. It was found, however, that conductive heat losses from the specimen to the ribbon subsequent to the pulse were important and could not be quantified sufficiently to permit an accurate determination of the thermal diffusivity. Step-function heating of the foil eliminated this difficulty. A number of problems arose in connection with the small size of our specimens. In the discussion to follow, we argue that experimental conditions have been established for reasonably accurate simultaneous determinations of thermal diffusivity and thermal conductivity in very small specimens. In addition, a novel data

reduction strategy based on a nonlinear least-squares analysis is presented.

2. IDEALIZATION

Equation (1) has the following exact solution⁸ for the semi-infinite region $x > 0$ upon imposition of a constant heat flux f_0 for $t > 0$ at $x = 0$:

$$T = T_0 + 2 \frac{f_0}{\lambda} \sqrt{\alpha t} \operatorname{ierfc} \left(\frac{x}{2\sqrt{\alpha t}} \right), \quad (2)$$

where $T = T_0$ for $t < 0$ at all x , and $T = T_0$ for all t at $x = \infty$. The complementary error-function integral is defined as⁸

$$\operatorname{ierfc}(z) \equiv \sqrt{\frac{1}{\pi}} e^{-z^2} - z \operatorname{erfc}(z), \quad (3)$$

and the complementary error function is defined as

$$\operatorname{erfc}(z) \equiv \frac{2}{\sqrt{\pi}} \int_z^\infty e^{-\xi^2} d\xi. \quad (4)$$

The thermal diffusivity α is defined by

$$\alpha \equiv \frac{\lambda}{\rho c_p}, \quad (5)$$

where λ is the thermal conductivity, ρ is the mass density, and c_p is the specific heat at constant pressure.

The experiment to simulate this theory must guarantee that the heat wave is one-dimensional at the temperature-sampling distance x , that the total specimen thickness is sufficiently large that the temperature at x is unchanged by further thickness increases, and that the heat flux entering the

specimen adequately approximates a mathematical step function. Additionally, instrumentation of the specimen to measure temperature transients at x must not jeopardize its monolithic quality and be adequately responsive. These issues are addressed in subsequent discussion.

3. EXPERIMENTAL ARRANGEMENT

Figure 1 is a cross-sectional schematic of the fixture developed to measure the thermal diffusivity and conductivity. Specimens are cut from solid cylindrical material of about 6.5-mm

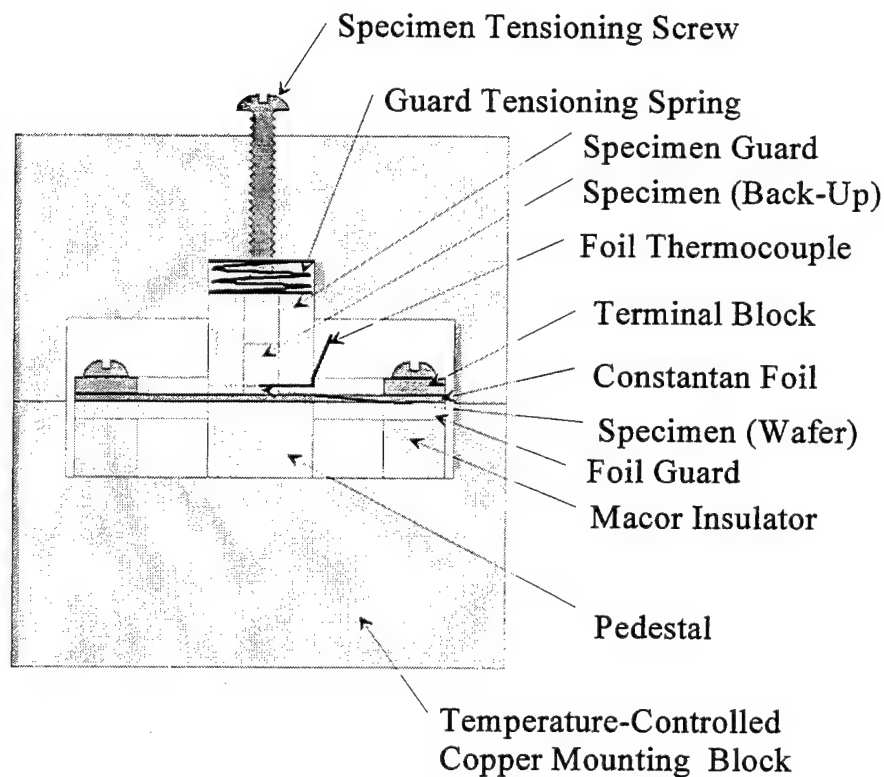


Figure 1. Schematic of thermal diffusivity/conductivity fixture in cross-sectional view.

diameter using a diamond-bladed, precision wafering saw. This saw operates at low speed using water as a cutting fluid, producing low-deformation cuts and variations in thickness for a single wafer of less than 1%. A complete specimen consists of a specimen wafer usually between 0.5 and 2.0 mm thick and a specimen back-up piece about 6.4 mm long. The thickness of the specimen wafer is measured with a micrometer which has a resolution of 0.0025 mm. Temperature is measured between the wafer and back-up piece by means of a bare Chromel/Alumel foil thermocouple of 0.005-mm thickness. Care is taken to place the thermocouple junction at the center of the wafer. The transient signal is amplified by a differential amplifier set to gain of 1,000 and captured by a digital oscilloscope. A typical trace consists of almost 2,000 data points.

On one of its sides the foil is in contact with the specimen wafer, and on the other it contacts an acrylic pedestal or base. In this respect our setup differs from that of Plummer, et al.,⁵ Harmathy,⁶ and Steere,⁷ all of whom placed specimen material on both sides of the foil in a symmetric arrangement. The pedestal, so long as it is sufficiently broad and thick, does not affect the functional dependence of the temperature on α , x , and t but does affect the dependence of the temperature on the specimen conductivity, λ . The mathematical solution for the case of the infinite composite solid is affected by the thermal diffusivity, α_b , and thermal conductivity, λ_b , of the pedestal or base material as follows:⁹

$$T = T_0 + \left(\frac{2f_0\lambda\sqrt{\alpha_b}}{\lambda\sqrt{\alpha_b} + \lambda_b\sqrt{\alpha}} \right) \sqrt{\alpha t} \operatorname{ierfc} \left(\frac{x}{2\sqrt{\alpha t}} \right) . \quad (6)$$

Equation (6) is the governing equation for this work. The heat flux f_0 generated in a foil of resistance R , length L , and width W through which a current I is passing is given by

$$f_0 = \frac{I^2 R}{LW} . \quad (7)$$

The foil employed here is 5- μm -thick Constantan,¹⁰ although 5- μm and 13- μm Manganin foils were also tested in the early development stages. Manganin has a somewhat lower resistivity temperature

coefficient but more readily tarnishes. Although we have no evidence that this thin oxide layer affects the experiment, it seemed prudent to avoid the issue by utilizing Constantan.

4. EXPERIMENTAL CONDITIONS FOR SATISFYING THE IDEALIZATION

In this section the extent to which the experiment conforms to the mathematical idealization embodied in Equation (6) is examined in detail.

4.1. Step-Function Flux

The mathematical ideality of the step-function heating stimulus is influenced by the finite rise time of the current in the foil and by the finite heat capacity of the foil. The rise time of the current was measured with a Pearson coil to be about 3 ms when switching was accomplished by a mercury-wetted relay, and no ringing was observed in the waveform at the edge of the step. With a total data-acquisition time of 4 s, such a rise time is seen to be very abrupt. A standard toggle switch was used initially, but the switching time was found to be about 30 ms and noisy, probably due to contact bounce. A regulated DC voltage supply provided power to the foil. The voltage drop across the foil proved constant to within about 0.1%. Thus, the step-function character of the *current* flowing in the foil would seem to be quite well approximated experimentally. However, even if the current were a perfect step function, the finite heat capacity of the foil results in a delay in achieving a constant heat flux into the specimen. This delay is longer for thicker foils, and its effect on the determination of diffusivity is greater the shorter the data acquisition time and the lower the diffusivity of the test specimen. An exact solution to this problem has been derived using Laplace transforms, and its impact on thermal diffusivity measurement discussed in detail elsewhere.¹¹ For our experimental conditions, this source of error results in less than a 2.5% underestimate of the diffusivity. As this error is smaller than the estimated accuracy of the technique developed here, no correction seems warranted although it is certainly feasible. One could also further minimize the effect by using even thinner foil.

An interesting problem arose in computing the heat flux by Equation (7). At first the flux was computed by measuring the voltage drop across the terminal blocks holding down the foil at each end. This voltage drop was then multiplied by the current flowing in the circuit to compute the power dissipated in the foil. Unfortunately, when the ratio of the diffusivity to the conductivity, both measured in the experiment, was compared to the product of independently measured density and specific heat as a consistency check (see Equation (5)), it was found that the former ratio was consistently about 20% smaller than the latter ratio. The accuracy of the ρc_p product was about 5%, and thus could not account for the discrepancy. This problem turned out to be due to electrical contact resistance between the terminal block and the foil. Measurements of the total resistance between terminal blocks (voltage drop across the terminal blocks divided by current) as a function of foil length are shown in Figure 2.

The intercept is the contact resistance, determined by the least-squares fit to be about 0.06Ω . Since the foil resistance for our standard 4.4 cm long foil is only 0.336Ω , about 15% of the power to the terminal blocks is dissipated by the contact resistance between terminal block and foil. The magnitude of this effect was not anticipated, and it proved difficult to diagnose. Once recognized, however, the problem was remedied by using in Equation (7) the actual foil resistance, which can be determined from the slope of the line in Figure 2. This problem was not encountered by Harmathy⁶ or Steere⁷ because of their much larger specimen (and therefore foil) sizes.

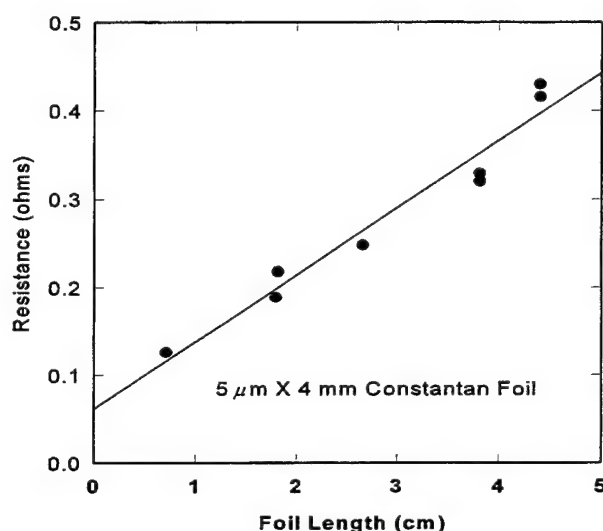


Figure 2. Measurements of total electrical resistance of series circuit containing Constantan foil and contact resistances between foil and terminal blocks for foils of varying lengths. Total electrical contact resistance is the y-intercept of the least-squares fit (solid line).

4.2. Uniformity of Flux

In addition to the temporal constraints on the heat flux, the mathematical idealization also presumes that the heat flux is spatially uniform (in the plane of the specimen surface) in order to assure one-dimensionality. A number of experimental details have a bearing on this issue. The foil used in our fixture is about 1.2 cm wide by 4.4 cm long, with the long dimension being the distance between the electrical terminal blocks. The terminal blocks are made of relatively massive (0.3 cm thick) flat copper bar stock and therefore act as a heat sink at the ends of the foil for heat generated along the length of the foil. If the length of the foil is too short, the flux into the specimen will not be spatially uniform due to temperature gradients at the ends of the foil in contact with the terminal blocks. One may address this problem by examining an exact solution for the limiting case of no heat loss from the surface of the foil and terminal-block temperatures maintained at ambient temperature. This case would be a poor assumption to make if one were trying to model the actual temperature distribution in the foil; however, such a case overestimates the heat conduction to the terminal blocks, thereby giving useful worst-case design guidance. The solution¹² for the temperature difference from ambient at some distance y from one end of a conductor of length L and thermal diffusivity α_c consists of the sum of a steady-state term and a transient term. Dividing this solution by the adiabatic solution gives the fraction, F , of the foil temperature at the given distance y that one would expect in the absence of heat loss to the terminal blocks, i.e.,

$$F = \frac{y(L-y)}{2\alpha_c t} - \frac{4L^2}{\pi^3\alpha_c t} \sum_{n=0}^{\infty} \frac{\exp\left[-\frac{\alpha_c(2n+1)^2\pi^2 t}{L^2}\right] \sin\left[\frac{(2n+1)\pi y}{L}\right]}{(2n+1)^3} \quad (8)$$

This fraction is plotted for a Constantan foil at several times in Figure 3. One can see that the assumption of temperature uniformity along the length of the foil becomes worse with time but is

quite good, even under our worst-case conditions, before 5 s in the center of the foil over the width of our specimen. Thus one may be quite assured of the flux uniformity along the length of the foil due to heat loss to the terminal blocks during our adopted data-acquisition period of 4 s.

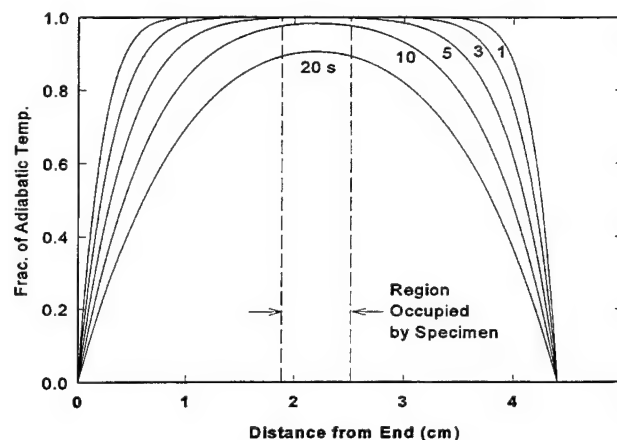


Figure 3. Worst-case calculations of nonuniformity in foil temperature due to heat losses to terminal blocks at the ends of the foil. Temperatures are expressed as a fraction of the temperature of the foil if there were no heat losses. Nonuniformities in foil temperature over the region occupied by the specimen will result in spatial nonuniformity of the heat flux, invalidating the mathematical idealization.

Edge effects across the width of the foil are another source of nonuniformity in the heat flux. Along a line perpendicular to the plane of the foil and through its center, the flux appears one-dimensional for distances

sufficiently close to the foil. At distances from the foil that are large compared with its width, the flux appears to emanate from a line source (assuming the foil is sufficiently long). We again examine this aspect by means of an exact solution for worst-case boundary conditions. Consider the temperature along a line perpendicular to and through the center of a circular disk from which a step-function heat flux emanates. Two-dimensionality in the resulting temperature field will clearly be evidenced at closer distances than in the case of the rectangular foil, making this a valid worst case. The solution for the temperature along the perpendicular through the center of the disk source¹³ ratioed with the one-dimensional solution (Equation (2)) is plotted in Figure 4. Results are shown for both acrylic and fused-quartz substrates. Deterioration of one-dimensionality occurs at much earlier times for acrylic, but at the end of our data-acquisition time of 3.6 s, the temperature at $x = 0.13$ cm is still 99% of the idealized one-dimensional value. Bearing in mind that this is a worst-case comparison, it is clear that foil edge effects can have but a negligible influence on results for our experimental conditions.

A third reason for spatial nonuniformity of the heat flux relates to the small size of the specimen itself. Our specimens are in the form of right circular cylinders with a diameter of about 6 mm. If the specimen is placed at the center of the foil, there is uncovered foil surrounding the specimen. This unbalanced boundary condition leads to temperature gradients in the plane of the foil radial to the axis of the specimen. This problem is remedied by the use of a guard material surrounding the specimen and covering

the foil up to the terminal blocks. In principle one should use a guard material with thermal properties identical to the specimen itself. In practice we have found that use of an acrylic guard results in acceptable accuracy for Pyrex glass, for example, which has a thermal diffusivity of about six times that of acrylic. Tests using an acrylic specimen wafer showed that the temperature difference from ambient after 5 s is only about 2% lower at the periphery of the specimen than at its center when a 5- μm -thick foil is covered by the guard. This result compares to temperature drops of 18% from center to edge of the specimen in the absence of a guard.

4.3. Semi-Infinite Specimen

The condition that the sample be sufficiently thick as to approximate being infinite may be determined as follows. The solution of Equation (1) for a slab of finite thickness l (and infinite lateral dimensions) subjected to step-function heating is¹⁴

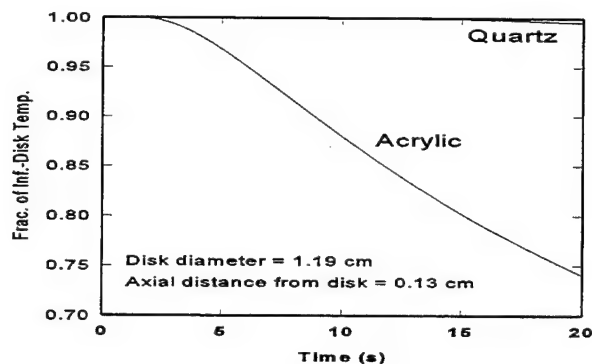


Figure 4. Worst-case calculations of departures from one-dimensionality of the temperature field in the specimen due to the finite width of the foil for two different specimen materials. Calculated is the temperature generated at a point along an axis through a disk source of diameter equal to the width of the foil. The results are displayed as a fraction of the temperature generated by a planar source of infinite extent.

$$T = T_0 + 2 \frac{f_0}{\lambda} \sqrt{\alpha t} \sum_{n=0}^{\infty} \left\{ \operatorname{ierfc} \left[\frac{2nl+x}{2\sqrt{\alpha t}} \right] + \operatorname{ierfc} \left[\frac{2(n+1)l-x}{2\sqrt{\alpha t}} \right] \right\} \quad (9)$$

For a given temperature-sampling station x_1 and a given experiment duration t_1 , there will be some minimum slab thickness l_1 beyond which the temperature at x_1 by Equation (2) will differ from that by Equation (9) by no more than, say, 1 %. For times earlier than t_1 the temperature differences between the two equations are even less than 1 %. Figure 5 illustrates the point quantitatively for $x_1 = 0.3$ mm and a 1 % criterion. If the diffusivity of the sample is 1.0×10^{-3} cm²/s and the data-acquisition time is 4 s, then by Figure 5 the minimum sample thickness l_1 required to satisfy the infinite-thickness boundary condition is a little over 1 mm. If either the time or the diffusivity is larger, then a thicker sample would be required. In this work the temperature-sampling distance x_1 is always less than 0.3 mm, the sample thickness is 6 mm or greater, and the data-acquisition time is 4 s. Thus, from the standpoint of sufficient sample thickness alone, the experimental setup is suitable for thermal diffusivities up to 0.2 cm²/s.

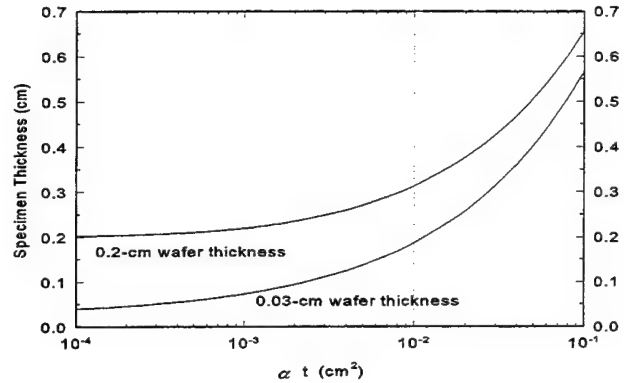


Figure 5. Calculations of the minimum thickness of a specimen (wafer + back-up piece) for which the temperature at a distance from the foil equal to the indicated wafer thickness differs from the temperature that would result from an infinite-thickness specimen by 1%. The figure shows, for example, that a total specimen thickness of 0.6 cm is sufficiently thick to approximate being infinitely thick in testing a material with a thermal diffusivity of 0.01 cm²/s if the data acquisition time is 10 s (or less). Vertical decade grid lines are shown for convenience.

D. Instrumentation Issues

At the outset of this study it was thought that the effects of thermal contact resistance might be significant at the specimen interface which includes the thermocouple and at the foil-specimen interface. In order to test the effects of contact resistance on the deduced value of diffusivity, three experiments were performed. In the first, an extra interface was introduced between the foil and the temperature-sampling station by stacking two wafers. The diffusivity was measured for this setup and compared to the value obtained using a single wafer of a thickness approximately the same as the combined thickness of the two wafers. In a series of five tests each, the difference in average values was not statistically significant (i.e., they differed by an amount less than or equal to the standard deviation of the mean). In the second experiment, an additional interface was introduced beyond the temperature-sampling station (i.e., at larger x). This modification, likewise, did not affect (in the same statistical sense as previously mentioned) the diffusivity values obtained in a five-test series. In the third experiment, conductive paste was used at each interface, but the diffusivity and conductivity results were unchanged (again relative to the standard deviation of the mean). These experiments prove that errors arising from thermal contact resistance in these low-diffusivity materials are insignificant. This same conclusion was reached by Shelley and Huber¹⁵ and by Steere⁷.

Another potential source of error is the adequacy of thermocouple response. A convenient way to address this problem is to compare results using two different thermocouple sizes. We found that Chromel/Alumel foil thermocouples, 5 μm and 12 μm thick, produced average diffusivity and conductivity values differing by statistically insignificant amounts. These tests were performed using the acrylic specimen in preference to fused quartz since the temperature gradients are higher in acrylic, resulting in greater sensitivity of the measurements to thermocouple response.

No measurable differences in diffusivity/conductivity could be attributed to variations in the specimen stack tension controlled by the tensioning screw at the top of the fixture. This tension was

normally set to bring the components into intimate contact without deforming or breaking the specimen components.

The magnitude of the heat flux is controlled by the voltage across the foil supplied by a regulated DC power supply. The choice of heat-flux magnitude was a compromise between a desire, on the one hand, to maximize the signal-to-noise ratio (improved by high fluxes) and the requirement of Equation (6), on the other hand, that the diffusivity and conductivity of the sample remain constant during measurement. A flux f_0 of about 0.25 watts/cm² was found to be an acceptable compromise between these limits, although a wide range of powers was found to be permissible.

The period of data acquisition is likewise a compromise between competing requirements. Short times are desirable to minimize radial heat losses and effects related to the finite length of the specimen, but long times are desirable from the standpoint of signal-to-noise ratio. The compromise adopted was 4 s, partitioned into an initial-temperature data period for the first 0.4 s and a heating phase lasting 3.6 s. This period is also consistent with the avoidance of nonuniform heat flux arising from the finite length and width of the foil as just discussed.

5. DATA ANALYSIS

A number of approaches might be taken to obtain a value for the thermal diffusivity from the measured temperature history between the specimen wafer and back-up piece. Plummer, et al.⁵ measured the ratio of the temperature at some x to that of the foil, then obtained the diffusivity graphically. Harmathy⁶ ratioed the temperature at a single position and at two different times, then found α graphically. The method of analysis used in the present work is based on the temperature measured at a single x but utilizes temperature data at all times during the experiment. This more comprehensive approach is enabled by performing a nonlinear least-squares fit^{16,17} of Equation (6) to the data using α and λ as fitting parameters. Because of noise in the data, it proved desirable to include T_0 in the list of fitting parameters rather than to input an averaged value. Likewise, to

minimize the effects of measurement imprecision in wafer thickness on the deduced value of diffusivity, five measurements were made of wafer thickness over its surface, and these values were included in the fitting process. In all cases the fitted values of T_0 and x were very close to their separately averaged values. In setting up the experiment, the digital oscilloscope's pretrigger function is selected at about -0.4 s. This results in the first N_{T_0} points being captured while the specimen is still at the initial temperature T_0 and the next N_T points captured during the constant heating phase at $t > 0$. If there are N_x wafer thickness measurements, then the fitting parameters, \hat{x} , $\hat{\alpha}$, $\hat{\lambda}$, and \hat{T}_0 , are varied until the variance of the fit σ_{fit}^2 , as given in the following equation, is minimized:

$$\sigma_{fit}^2 = \sum_{i=1}^{N_T} w_i^T (T_i - T(\hat{x}, \hat{\alpha}, \hat{\lambda}; t_i))^2 + \sum_{i=1}^{N_{T_0}} w_i^T (T_{0_i} - \hat{T}_0)^2 + \sum_{i=1}^{N_x} w_i^x (x_i - \hat{x})^2 \quad (10)$$

The weights are defined as the reciprocal of the respective parameter measurement variances, which are determined from experience. Note that this approach is not equivalent to inverting Equation (6) for α and λ using the average values of x and T_0 . Not only are optimum values of α and λ obtained, consistent with the assumption of random error in the measurement of T , T_0 , and x , but a more accurate estimate of the standard deviation in the fitted parameters is also available, which properly reflects the propagation of measurement errors through the nonlinear governing equation. Figure 6 illustrates a typical

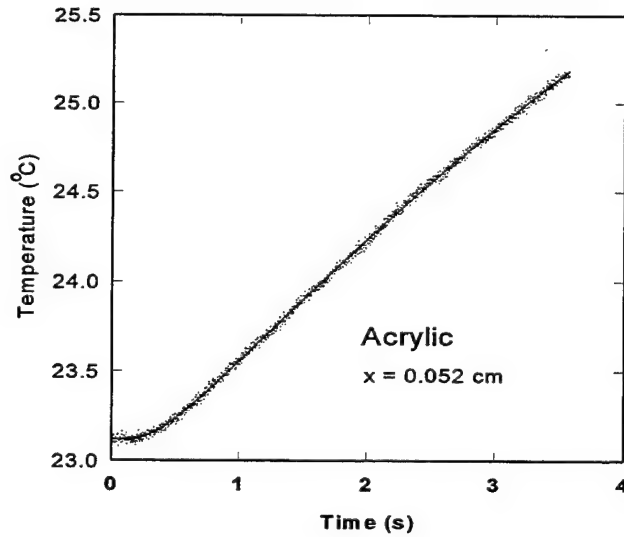


Figure 6. Typical experimental temperature data (points) measured for an acrylic (PMMA) specimen at a distance of 0.052 cm from the foil compared with the theoretical temperature (solid curve) computed from Equation (6) with the optimized values for thermal conductivity and diffusivity.

comparison between Equation (6), evaluated using the least-squares values of α , λ , x , and T_0 , and the experimental data. The quality of the fit is seen to be excellent.

6. DIFFUSIVITY RESULTS

The technique just described was applied to samples of acrylic, Pyrex glass, and fused quartz at room temperature. The acrylic, poly(methylmethacrylate) or PMMA, was the same material from which the guard components were fabricated. The results for these materials compared with literature values are given in Table 1.

Fused quartz comes as close as any material to being a standard reference material in the lower conductivity range. In fact, the TPRC compendium¹⁸ compiles enough data on the thermal conductivity of fused quartz to provide a set of recommended values, to an accuracy estimated as $\pm 3\%$, through the temperature range of interest in this study. The subsequent work of Sugawara¹⁹ claims to have measured the thermal conductivity of very pure fused quartz to an accuracy of $\pm 1.5\%$. The values of diffusivity in Table 1 attributed to these two sources are obtained using our measured values of the density and specific heat of the fused-quartz specimen, viz., $\rho = 2.194 \text{ g/cm}^3$ and $c_p = 0.175 \text{ cal/g-K}$ at 296 K. The present technique yields a value for the conductivity of fused quartz about 13% lower than those of the TPRC¹⁸ and Sugawara¹⁹. The sample of fused quartz tested here is the lowest grade material manufactured by Heraeus Amercil (T08 Commercial Rod). It is not known to what extent its chemical impurity and bubble inclusions are responsible for the shortfall in conductivity just noted; however, Sugawara¹⁹ identified sample purity as an important factor in the $\pm 8\%$ variation in conductivity values among different researchers. The tolerance values attached to our values are indicative of the precision of our measurement and are one standard deviation of the mean, typically of five separate runs.

Our measurements of the thermal conductivity for Pyrex glass (Corning #7740) differ by only 3% from the TPRC recommended values, lending confidence to our values and reinforcing suspicion

that impurities in our fused-quartz specimen may be responsible for the relatively unfavorable comparison to the TPRC¹⁸ values for that material.

**TABLE 1. Results of Present Technique Compared to
Published Work on Similar Materials**

TEST MATERIAL	$10^3 \times \alpha$ (cm ² /s)	$10^4 \times \lambda$ (cal/cm-s-K)	REFERENCE
acrylic (PMMA)	$1.14 \pm .02$ @ 296 K	$4.29 \pm .05$ @ 296 K	this work
"	1.28 @ 296 K [†]	-	Luikov, et al. ²⁰
"	1.13 @ 298 K	4.58 @ 298 K	Krischer & Esdorn ²¹
"	0.948^{\dagger} @ 296 K [‡]	3.64 @ 296 K [‡]	Lucks, et al. ²⁶
"	1.24^{\dagger} @ 313 K	4.61 @ 313 K	Brown & Otten ²²
"	1.22^{\dagger} @ 293 K	4.52 @ 293 K	Eiermann ²³
Pyrex	$6.45 \pm .22$ @ 296 K	25.4 ± 1.3 @ 296 K	this work
"	-	26.2 @ 296 K [‡]	TPRC ¹⁸ recommend.
"	5.5 @ 298 K	-	Plummer, et al. ⁵
"	5.75 @ 298 K	23.9 @ 298 K	Hasselman, et al. ²⁴
fused quartz	$7.72 \pm .10$ @ 296 K	28.6 ± 1.1 @ 296 K	this work
"	8.54^{\dagger} @ 295 K [‡]	32.8 @ 296 K [‡]	TPRC ¹⁸ recommend.
"	8.65^{\dagger} @ 295 K [‡]	33.2 @ 296 K [‡]	Sugawara ¹⁹
"	8.33 @ 296 K [‡]	-	Luikov, et al. ²⁰
"	-	28.2 @ 314 K	Ballard, et al. ²⁵

[†] Computed from our measured value of ρc_p using Equation (5).

[‡] Value at this temperature obtained by linear interpolation.

The literature values of α and λ for acrylic are more widely scattered and difficult to assess. No recommended values are offered in the TPRC¹⁸ compendium. Although the references quoted

for acrylic are not comprehensive, we note that our value is almost exactly the average of the quoted literature values. If the possibly anomalous value of Lucks, et al.²⁶ is omitted, our measured conductivity is 6% lower than the resulting average literature value. In computing the diffusivity for acrylic from published values of the thermal conductivity, we have used our measurements of the density and specific heat, $\rho = 1.181 \text{ g/cm}^3$ and $c_p = 0.315 \text{ cal/g-K}$ at 296 K.

Using our independent measurements of the mass density (estimated accuracy = 1%) and specific heat (estimated accuracy = 5%) for our acrylic and fused-quartz specimens, determined by dimensional measurement/weighing and differential scanning calorimetry, respectively, the self-consistency between diffusivity and conductivity yielded by the present experiment may be tested. For example, the measured value of conductivity differs from that computed from Equation (5) by 3% or less for acrylic and fused quartz. Taking all of the aforementioned comparisons into account, we therefore feel justified in claiming an accuracy of about 5% in measurements of the thermal diffusivity and conductivity by the present technique for materials falling into the range between acrylic and Pyrex glass. This same accuracy may also apply to fused quartz; however, it would be prudent to prove this by testing a specimen of purity comparable to that of Sugawara¹⁹. The solid-propellant materials which motivated this work fall quite generally in the more restricted range and therefore may suitably be studied using this technique.

INTENTIONALLY LEFT BLANK

7. REFERENCES

1. Tye, R. P. (editor). Thermal Conductivity. Vol. 1, London: Academic Press, 1969.
2. Parker, W. J., R. J. Jenkins, C. P. Butler, and G. L. Abbott. Journal of Applied Physics, vol. 32, p. 1679, 1961.
3. Clark, L. M., and R. E. Taylor. Journal of Applied Physics. Vol. 46, p. 714, 1975.
4. Chen, F. C., Y. M. Poon, and C. L. Choy. Polymer. Vol. 18, p. 129, 1977.
5. Plummer, W. A., D. E. Plummer, and A. A. Comstock. J. Am. Ceram. Soc. Vol. 45, p. 310, 1962.
6. Harmathy, T. Z. Journal of Applied Physics. Vol. 35, p. 1190, 1964.
7. Steere, R. C. Journal of Applied Physics. Vol. 37, p. 3338, 1966.
8. Carslaw, H. S., and J. C. Jaeger. Conduction of Heat in Solids. 2nd ed., London: Oxford University Press, p. 75, 1959.
9. Carslaw, H. S., and J. C. Jaeger, op. cit., p.88.
10. Constantan foil was kindly supplied by Hamilton Precision Metals, Lancaster, PA.
11. Miller, M. S. Journal of Applied Physics. Vol. 72, p. 3904, 1992.
12. Carslaw, H. S., and J. C. Jaeger. Operational Methods in Applied Mathematics. 2nd ed., London: Oxford University Press, section 52, 1948.
13. Carslaw, H. S., and J. C. Jaeger. Conduction of Heat in Solids. London: Oxford University Press, equation 10.5 (5), 1959.
14. Carslaw, H. S., and J. C. Jaeger, op. cit, p. 112.
15. Shelly, D. L., and S. F. Huber. "Thermal Diffusivity of Poly(tetraflouroethylene) between 140° and 125° C." Thermal Conductivity, Proceedings of the Eighth Conference, edited by C. Y. Ho and R. E. Taylor, New York: Plenum Press, 1969.
16. Wentworth, W. E. Journal of Chemical Education. Vol. 42, p. 96, 1965.
17. Marquardt, D. W. J. Soc. Indust. Appl. Math. Vol. 11, p. 431, 1963.

18. Touloukian, Y. S., R. W. Powell, C. Y. Ho, and P. G. Klemens (eds.). Thermophysical Properties of Matter: Vol. 2, Thermal Conductivity of Nonmetallic Solids. New York: IFI Plenum.
19. Sugawara, A. Journal of Applied Physics. Vol. 39, p. 5994, 1968.
20. Luikov, A. V., L. L. Vasiliev, and A. G. Shashkov. Proc. 3rd ASME Symp. on Thermophysical Properties, p. 314, 1965.
21. Krischer, O., and H. Esdorn. VDI-Forschungs-Heft. Vol. 21 (450B), p. 28, 1955.
22. Brown, R. B., and L. Otten. Int. Journal of Thermophysics. Vol. 9, p. 1131, 1988.
23. Eiermann, K. Kunststoffe. Vol. 51, p. 512, 1961.
24. Hasselman, D. P. H., and W. A. Zdaniewski. J. Mat. Sci. Vol. 15 (Letters), p. 518, 1980.
25. Ballard, S. S. K. A. McCarthy, and W. C. Davis. Rev. Sci. Inst. Vol. 21, p. 905, 1950.
26. Lucks, C. F., G. F. Bing, J. Matolich, H. W. Deem, and H. B. Thompson. USAF TR 6145, 1952. (AD95239)

<u>NO. OF COPIES</u>	<u>ORGANIZATION</u>
2	DEFENSE TECHNICAL INFO CTR ATTN DTIC DDA 8725 JOHN J KINGMAN RD STE 0944 FORT BELVOIR VA 22060-6218
1	HQDA DAMO FDQ ATTN DENNIS SCHMIDT 400 ARMY PENTAGON WASHINGTON DC 20310-0460
1	US MILITARY ACADEMY MATH SCI CTR OF EXCELLENCE DEPT OF MATHEMATICAL SCI ATTN MDN A MAJ DON ENGEN THAYER HALL WEST POINT NY 10996-1786
1	DIRECTOR US ARMY RESEARCH LAB ATTN AMSRL CS AL TP 2800 POWDER MILL RD ADELPHI MD 20783-1145
1	DIRECTOR US ARMY RESEARCH LAB ATTN AMSRL CS AL TA 2800 POWDER MILL RD ADELPHI MD 20783-1145
3	DIRECTOR US ARMY RESEARCH LAB ATTN AMSRL CI LL 2800 POWDER MILL RD ADELPHI MD 20783-1145
<u>ABERDEEN PROVING GROUND</u>	
2	DIR USARL ATTN AMSRL CI LP (305)

NO. OF COPIES	ORGANIZATION
4	NATIONAL BUREAU OF STANDARDS US DEPARTMENT OF COMMERCE ATTN J HASTIE M JACOX T KASHIWAGI H SEMERJIAN WASHINGTON DC 20234
1	OSD/SDIO/IST ATTN L CAVENY PENTAGON WASHINGTON DC 20301-7100
2	HQDA SARD TT DR F MILTON MR J APPEL WASH DC 20310-0103
1	HQDA OASA RDA ATTN DR C H CHURCH PENTAGON ROOM 3E486 WASH DC 20310-0103
5	CDR ARO ATTN R GHIRARDELLI D MANN R SINGLETON R SHAW AMXRO RT IP LIBRARY SERVICES PO BOX 12211 RSCH TRIANGLE PARK NC 27709-2211
3	CDR ARDEC ATTN SMCAR AEE B D S DOWNS SMCAR AEE BR L HARRIS SMCAR AEE J A LANNON PICATINNY ARSENAL NJ 07806-5000
1	DIRECTOR US ARMY BENET LABORATORY ATTN SMCAR CCB B SAM SOPOK WATERVALIET NY 12189
2	CDR MICOM ATTN AMSMI RD PR E A R MAYKUT AMSMI RD PR P R BETTS REDSTONE ARSENAL AL 35898-5000
1	OFFICE OF NAVAL RESEARCH DEPARTMENT OF THE NAVY ATTN R S MILLER CODE 432 800 N QUINCY STREET ARLINGTON, VA 22217

NO. OF COPIES	ORGANIZATION
1	CDR NAVAL AIR SYSTEMS CMD ATTN J RAMNARACE AIR-54111C WASHINGTON DC 20360
2	CDR NAVAL SURFACE WARFARE CTR ATTN R BERNECKER R-13 G B WILMOT R-16 SILVER SPRING MD 20903-5000
5	CDR NAVAL RESEARCH LABORATORY ATTN M C LIN J MCDONALD E ORAN J SHNUR R J DOYLE CODE 6110 WASHINGTON DC 20375
2	CDR NAVAL WEAPONS CTR ATTN T BOGGS CODE 388 T PARR CODE 3895 CHINA LAKE CA 93555-6001
1	SUPERINTENDENT NAVAL POSTGRADUATE SCHOOL DEPT OF AERONAUTICS ATTN D W NETZER MONTEREY CA 93940
3	AL/LSCF ATTN R CORLEY R GEISLER J LEVINE EDWARDS AFB CA 93523-5000
1	AFOSR ATTN J M TISHKOFF BOLLING AFB WASHINGTON DC 20332
1	CMDT USAFAS ATTN ATSF TSM CN FORT SILL OK 73503-5600
1	UNIV OF DAYTON RSCH INSTITUTE ATTN D CAMPBELL AL/PAP EDWARDS AFB CA 93523
1	NASA LANGLEY RESEARCH CENTER LANGLEY STATION ATTN G B NORTHAM MS 168 HAMPTON VA 23365

NO. OF COPIES	ORGANIZATION
1	DIR LANL ATTN B NICHOLS T7 MS-B284 PO BOX 1663 LOS ALAMOS NM 87545
2	DIR LLNL ATTN C WESTBROOK W TAO MS L282 PO BOX 808 LIVERMORE CA 94550
3	DIR SNL DIVISION 8354 ATTN S JOHNSTON P MATTERN D STEPHENSON LIVERMORE CA 94550
1	BRIGHAM YOUNG UNIV DEPT OF CHEMICAL ENGINEERING ATTN M W BECKSTEAD PROVO UT 84058
1	CA INSTITUTE OF TECHNOLOGY JET PROPULSION LABORATORY ATTN L STRAND MS 125-224 4800 OAK GROVE DRIVE PASADENA CA 91109
1	CA INSTITUTE OF TECHNOLOGY ATTN F E C CULICK MC 301-46 204 KARMAN LAB PASADENA CA 91125
1	CORNELL UNIV DEPARTMENT OF CHEMISTRY ATTN T A COOL BAKER LABORATORY ITHACA NY 14853
3	GA INST OF TECHNOLOGY SCHOOL OF AEROSPACE ENGINEERING ATTN E PRICE W C STRAHLE B T ZINN ATLANTA GA 30332
1	THE JOHNS HOPKINS UNIV CHEMICAL PROPULSION INFO AGENCY ATTN T W CHRISTIAN 10630 LITTLE PATUXENT PKWY STE 202 COLUMBIA MD 21044-3200

NO. OF COPIES	ORGANIZATION
4	PENNSYLVANIA STATE UNIV DEPT OF MECHANICAL ENGINEERING ATTN K KUO M MICCI S THYNELL V YANG UNIVERSITY PARK PA 16802
2	PRINCETON UNIVERSITY FORRESTAL CAMPUS LIBRARY ATTN K BREZINSKY I GLASSMAN PO BOX 710 PRINCETON NJ 08540
1	PURDUE UNIVERSITY SCHOOL OF AERONAUTICS & ASTRONAUTICS ATTN J R OSBORN GRISSOM HALL WEST LAFAYETTE IN 47906
1	PURDUE UNIVERSITY DEPT OF CHEMISTRY ATTN E GRANT WEST LAFAYETTE, IN 47906
2	PURDUE UNIVERSITY SCHOOL OF MECH ENGINEERING ATTN N M LAURENDEAU S N B MURTHY TSPC CHAFFEE HALL WEST LAFAYETTE IN 47906
1	RENSSELAER POLYTECHNIC INST DEPT OF CHEMICAL ENGINEERING ATTN A FONTIJN TROY NY 12181
1	STANFORD UNIVERSITY DEPT OF MECH ENGINEERING ATTN R HANSON STANFORD CA 94305
1	UNIV OF CALIFORNIA LOS ALAMOS SCIENTIFIC LAB PO BOX 1663 MS B216 LOS ALAMOS NM 87545
1	UNIV OF CA-BERKELEY CHEMISTRY DEPARMENT ATTN C BRADLEY MOORE 211 LEWIS HALL BERKELEY CA 94720

NO. OF
COPIES ORGANIZATION

1 UNIV OF CA SAN DIEGO
ATTN F A WILLIAMS
AMES B010
LA JOLLA CA 92093

2 UNIV OF CA SANTA BARBARA
QUANTUM INSTITUTE
ATTN K SCHOFIELD
M STEINBERG
SANTA BARBARA CA 93106

1 UNIV OF CO AT BOULDER
ENGINEERING CENTER
ATTN J DAILY
CAMPUS BOX 427
BOULDER CO 80309-0427

1 UNIV OF DELAWARE
ATTN T BRILL
CHEMISTRY DEPARTMENT
NEWARK DE 19711

1 UNIV OF FLORIDA
DEPT OF CHEMISTRY
ATTN J WINEFORDNER
GAINESVILLE FL 32611

1 UNIV OF ILLINOIS
DEPT OF MECH ENG
ATTN H KRIER
144MEB 1206 W GREEN ST
URBANA IL 61801

1 UNIV OF MICHIGAN
GAS DYNAMICS LAB
AEROSPACE ENGINEERING BLDG
ATTN G M FAETH
ANN ARBOR MI 48109-2140

1 UNIV OF MINNESOTA
DEPT OF MECH ENGINEERING
ATTN E FLETCHER
MINNEAPOLIS MN 55455

3 UNIV OF SOUTHERN CA
DEPT OF CHEMISTRY
ATTN R BEAUDET
S BENSON
C WITTIG
LOS ANGELES CA 90007

NO. OF
COPIES ORGANIZATION

1 UNIVERSITY OF TEXAS
DEPT OF CHEMISTRY
ATTN W GARDINER
AUSTIN TX 78712

1 VA POLYTECHNIC INST & STATE UNIV
ATTN J A SCHETZ
BLACKSBURG VA 24061

8 ALLIANT TECHSYSTEMS INC
MARINE SYSTEMS GROUP
ATTN R BECKER
J BODE
D E BRODEN MS MN50-2000
R BURETTA
C CANDLAND
L OSGOOD
M SWENSON
R E TOMPKINS MN 11-2720
600 2ND STREET NE
HOPKINS MN 55343

1 APPLIED COMBUSTION TECH INC
ATTN A M VARNEY
PO BOX 607885
ORLANDO FL 32860

2 APPLIED MECHANICS REVIEWS
THE AMERICAN SOCIETY OF MECH ENGINEERS
ATTN R E WHITE
A B WENZEL
345 E 47TH STREET
NEW YORK NY 10017

1 BATTELLE
TWSTIAC HUGGINS
505 KING AVENUE
COLUMBUS OH 43201-2693

1 COHEN PROFESSIONAL SERVICES
ATTN N S COHEN
141 CHANNING STREET
REDLANDS CA 92373

1 EXXON RESEARCH & ENG CO
ATTN A DEAN
ROUTE 22E
ANNANDALE NJ 08801

1 FREEDMAN ASSOCIATES
ATTN E FREEDMAN
2411 DIANA ROAD
BALTIMORE MD 21209-1525

NO. OF
COPIES ORGANIZATION

1 GE ORDNANCE SYSTEMS
ATTN J MANDZY
100 PLASTICS AVENUE
PITTSFIELD MA 01203

1 GENERAL APPLIED SCIENCE LABS INC
77 RAYNOR AVENUE
RONKONKAMA NY 11779-6649

1 GENERAL MOTORS RSCH LABS
PHYSICAL CHEMISTRY DEPARTMENT
ATTN T SLOANE
WARREN MI 48090-9055

2 HERCULES INC
ALLEGHENY BALLISTICS LAB
ATTN W B WALKUP
E A YOUNT
PO BOX 210
ROCKET CENTER WV 26726

1 HERCULES INC
ATTN R V CARTWRIGHT
100 HOWARD BLVD
KENVIL NJ 07847

1 HUGHES AIRCRAFT COMPANY
ATTN T E WARD
8433 FALLBROOK AVENUE
CANOGA PARK CA 91303

1 IBM CORPORATION
RESEARCH DIVISION
ATTN A C TAM
5600 COTTLE ROAD
SAN JOSE CA 95193

1 IIT RESEARCH INSTITUTE
ATTN R F REMALY
10 WEST 35TH STREET
CHICAGO IL 60616

1 LOCKHEED MISSILES & SPACE CO
DEPT 52-35 B204 2
ATTN GEORGE LO
3251 HANOVER STREET
PALO ALTO CA 94304

1 OLIN ORDNANCE
ATTN V MCDONALD LIBRARY
PO BOX 222
ST MARKS FL 32355-0222

NO. OF
COPIES ORGANIZATION

1 PAUL GOUGH ASSOCIATES INC
ATTN P S GOUGH
1048 SOUTH STREET
PORTSMOUTH NH 03801-5423

2 PRINCETON COMB RSCH LABS INC
ATTN N A MESSINA
M SUMMERFIELD
PRINCETON CORPORATE PLAZA
BLDG IV SUITE 119
11 DEERPARK DRIVE
MONMOUTH JUNCTION NJ 08852

1 ROCKWELL INTERNATIONAL CORP
ROCKETDYNE DIVISION
ATTN J E FLANAGAN HB02
6633 CANOGA AVENUE
CANOGA PARK CA 91304

1 SCIENCE APPLICATIONS INC
ATTN R B EDELMAN
23146 CUMORAH CREST
WOODLAND HILLS CA 91364

3 SRI INTERNATIONAL
ATTN G SMITH
D CROSLEY
D GOLDEN
333 RAVENSWOOD AVENUE
MENLO PARK CA 94025

1 STEVENS INSTITUTE OF TECH
DAVIDSON LABORATORY
ATTN R MCALEVY III
HOBOKEN NJ 07030

2 SVERDRUP TECHNOLOGY INC
LERC GROUP
ATTN R J LOCKE MS SVR-2
J DEUR
2001 AEROSPACE PARKWAY
BROOK PARK OH 44142

1 TEXTRON DEFENSE SYSTEMS
ATTN A PATRICK
2385 REVERE BEACH PARKWAY
EVERETT MA 02149-5900

NO. OF
COPIES ORGANIZATION

3 THIOKOL CORPORATION
ELKTON DIVISION
ATTN R BIDDLE
R WILLER
TECH LIB
PO BOX 241
ELKTON MD 21921

3 THIOKOL CORPORATION
WASATCH DIVISION
ATTN S J BENNETT
PO BOX 524
BRIGHAM CITY UT 84302

1 UNITED TECHNOLOGIES CORP
CHEMICAL SYSTEMS DIVISION
ATTN R R MILLER
PO BOX 49028
SAN JOSE CA 95161-9028

1 UNITED TECHNOLOGIES RSCH CTR
ATTN A C ECKBRETH
EAST HARTFORD CT 06108

1 UNIVERSAL PROPULSION COMPANY
ATTN H J MCSPADDEN
25401 NORTH CENTRAL AVENUE
PHOENIX AZ 85027-7837

1 VERITAY TECHNOLOGY INC
ATTN E B FISHER
4845 MILLERSPORT HIGHWAY
PO BOX 305
EAST AMHERST NY 14051-0305

NO. OF
COPIES ORGANIZATION

41 DIR USARL
ATTN AMSRL WMP
G F ADAMS
W R ANDERSON
R A BEYER
K P MC-NEILL BOONSTOPPEL
S W BUNTE
C F CHABALOWSKI
A COHEN
R CUMPTON
R DANIEL
D DEVYNCK
R A FIFER
B E FORCH
J M HEIMERL
B E HOMAN
A W HORST
A JUHASZ
A J KOTLAR
R KRANZE
E LANCASTER
W F MCBRATNEY
K L MCNESBY
M MCQUAID
N E MEAGHER
M S MILLER
A W MIZIOLEK
J B MORRIS
J E NEWBERRY
S V PAI
R A PESCE-RODRIGUEZ
J RASIMAS
P REEVES
B M RICE
P SAEGAR
R C SAUSA
M A SCHROEDER
R SCHWEITZER
L D SEGER
J A VANDERHOFF
D VENIZELOS
A WHREN
H L WILLIAMS

REPORT DOCUMENTATION PAGE			Form Approved OMB No. 0704-0188	
<small>Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project(0704-0188), Washington, DC 20503.</small>				
1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE March 1997		3. REPORT TYPE AND DATES COVERED Final, 15 Jan 92 - 1 Jun 93
4. TITLE AND SUBTITLE A New Technique for the Simultaneous Measurement of Thermal Diffusivity and Thermal Conductivity of Small Energetic-Material Specimens			5. FUNDING NUMBERS PR: 1L161102AH43	
6. AUTHOR(S) Martin S. Miller and Anthony J. Kotlar				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) U.S. Army Research Laboratory ATTN: AMSRL-WM-PC Aberdeen Proving Ground, MD 21005-5066			8. PERFORMING ORGANIZATION REPORT NUMBER ARL-TR-1321	
9. SPONSORING/MONITORING AGENCY NAMES(S) AND ADDRESS(ES)			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES This report was also published in Review of Scientific Instruments, vol. 64, pp. 2954-2960, 1993.				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) An experimental technique to simultaneously measure the thermal diffusivity and thermal conductivity of small specimens of thermal-insulator materials is described. Experimental conditions that approach the mathematical idealization of a one-dimensional, infinite, two-component, composite solid whose planar interface is subjected to a step-function heat flux are developed. The heat flux is generated by resistive heating of a thin metallic foil. Although this principle has been exploited previously, the present technique permits specimens with volumes two orders of magnitude smaller than prior work based on the same idealization. A number of difficulties related to small specimen volume are identified and overcome. Another improvement over past efforts is the use of nonlinear least-squares analysis to determine the optimum values for diffusivity and conductivity. A comparison of measurements of these properties for acrylic and Pyrex glass with literature values suggests that the technique affords accuracies of about 5% for materials in this range.				
14. SUBJECT TERMS thermal conductivity, thermal diffusivity, energetic materials, propellant			15. NUMBER OF PAGES 31	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED	18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED	19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED	20. LIMITATION OF ABSTRACT UL	

INTENTIONALLY LEFT BLANK.

USER EVALUATION SHEET/CHANGE OF ADDRESS

This Laboratory undertakes a continuing effort to improve the quality of the reports it publishes. Your comments/answers to the items/questions below will aid us in our efforts.

1. ARL Report Number/Author ARL-TR-1321 (Miller) Date of Report March 1997

2. Date Report Received _____

3. Does this report satisfy a need? (Comment on purpose, related project, or other area of interest for which the report will be used.) _____

4. Specifically, how is the report being used? (Information source, design data, procedure, source of ideas, etc.) _____

5. Has the information in this report led to any quantitative savings as far as man-hours or dollars saved, operating costs avoided, or efficiencies achieved, etc? If so, please elaborate. _____

6. General Comments. What do you think should be changed to improve future reports? (Indicate changes to organization, technical content, format, etc.) _____

CURRENT
ADDRESS

Organization

Name

E-mail Name

Street or P.O. Box No.

City, State, Zip Code

7. If indicating a Change of Address or Address Correction, please provide the Current or Correct address above and the Old or Incorrect address below.

OLD
ADDRESS

Organization

Name

Street or P.O. Box No.

City, State, Zip Code

(Remove this sheet, fold as indicated, tape closed, and mail.)
(DO NOT STAPLE)

DEPARTMENT OF THE ARMY

OFFICIAL BUSINESS

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 0001,APG,MD

POSTAGE WILL BE PAID BY ADDRESSEE

DIRECTOR
US ARMY RESEARCH LABORATORY
ATTN AMSRL WM PC
ABERDEEN PROVING GROUND MD 21005-5066



NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES

